


dBm Ref Level : -62 dBm
Ref Offset : 0.0 dB

Block 944

Detector : Auto Peak (Auto)
Trigger Mode : Free Run
Trace : Clear / Write

RBW : 1 MHz
VBW : 300 Hz
SWT : 100 ms

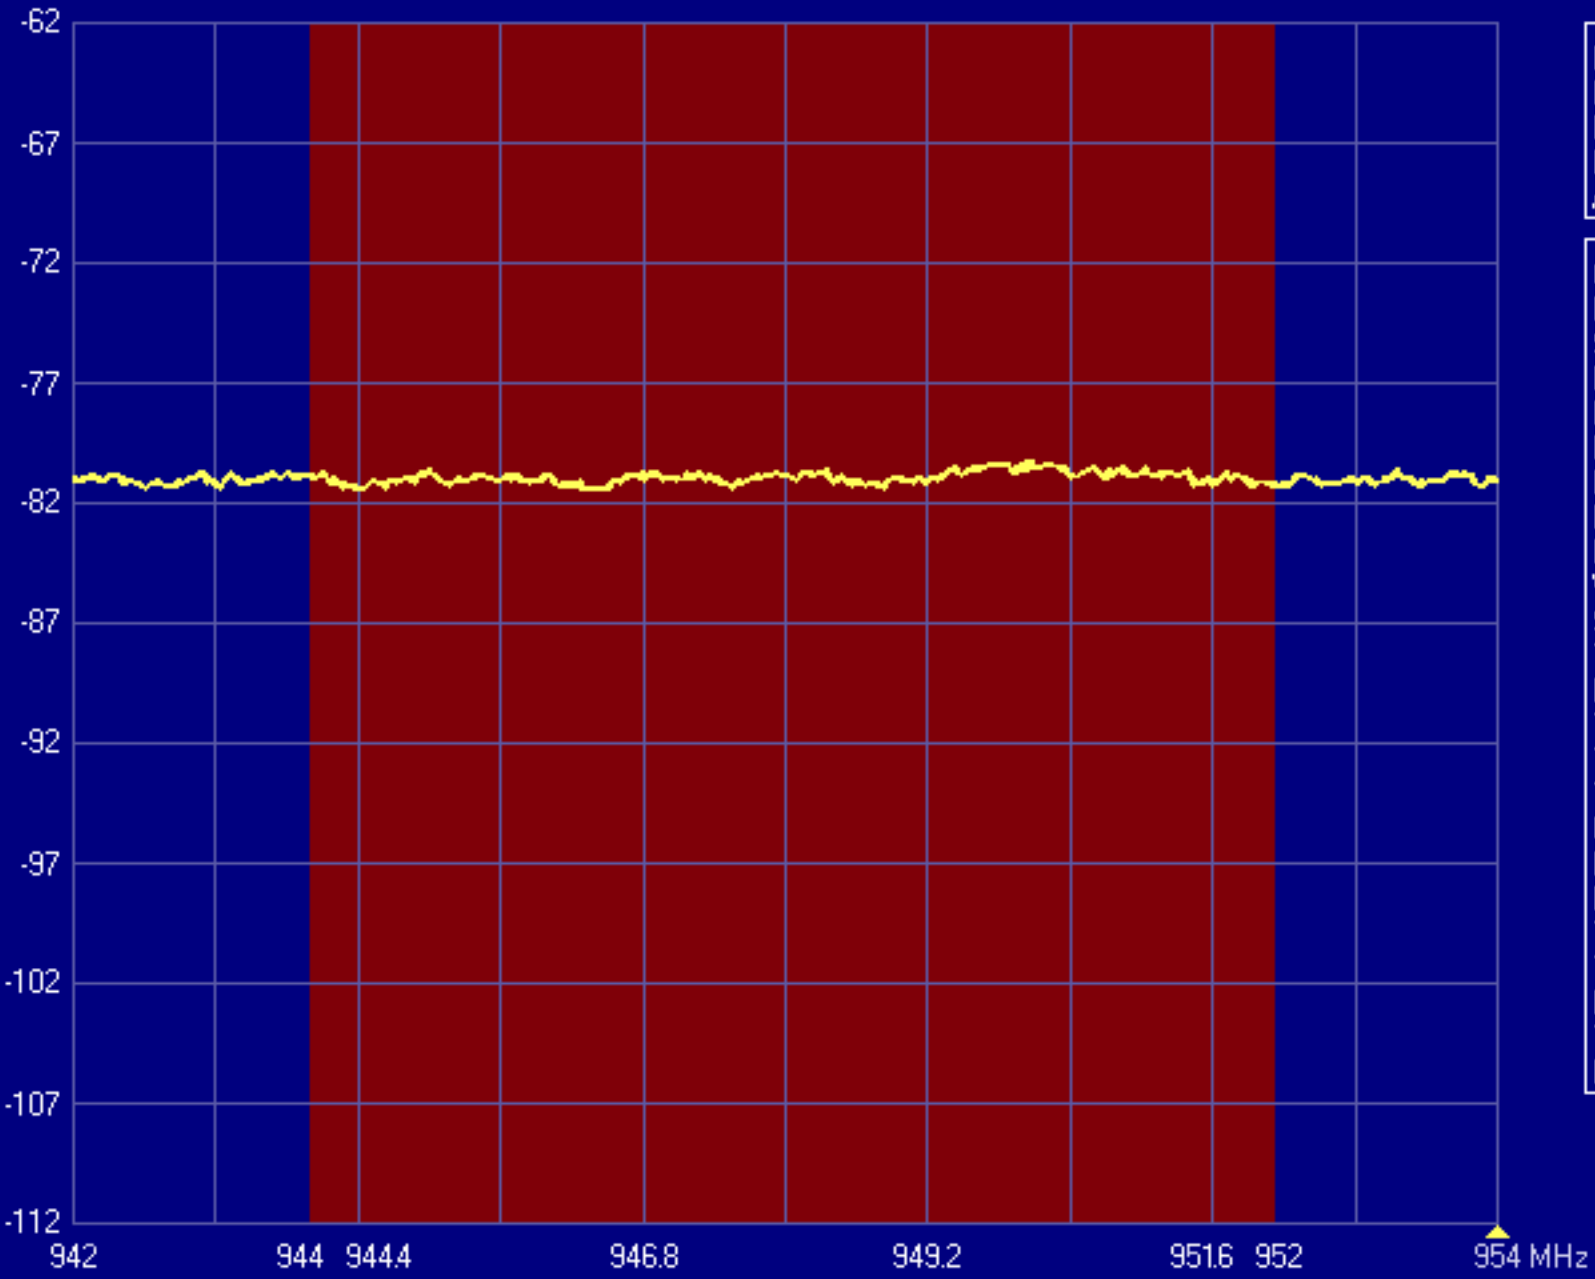

Trace	
Name	: Analyzer
Ref Level	: -62 dBm
Range	: 5 dB/div
Result	: ---
Averaging	: ---

Status	
Center Frequency	: 948 MHz
Frequency Offset	: 0 Hz
Span	: 12 MHz
Ref Offset	: 0.0 dB
RF Attenuator	: 0 dB
Preamplifier	: Off
Dynamic Range	: Low Distortion
RF Input	: 50 Ohm
RBW	: 1 MHz
VBW	: 300 Hz
SWT	: 100 ms
Trace Mode	: Clear / Write
Detector	: Auto Peak (Auto)
Trigger Mode	: Free Run
Trigger Level	: ---
Trigger Delay	: ---
Upper Limit	: ---
Lower Limit	: ---
External Reference	: Disabled
Transducer	: ---
Transducer (dB)	: ---
Date	: 4/12/2006
Time	: 11:26:59 AM
Instrument	: FSH03 - 103116

Start Frequency : 942 MHz Stop Frequency : 954 MHz
Center Frequency : 948 MHz Span : 12 MHz

Analyzer